

FIG. 1


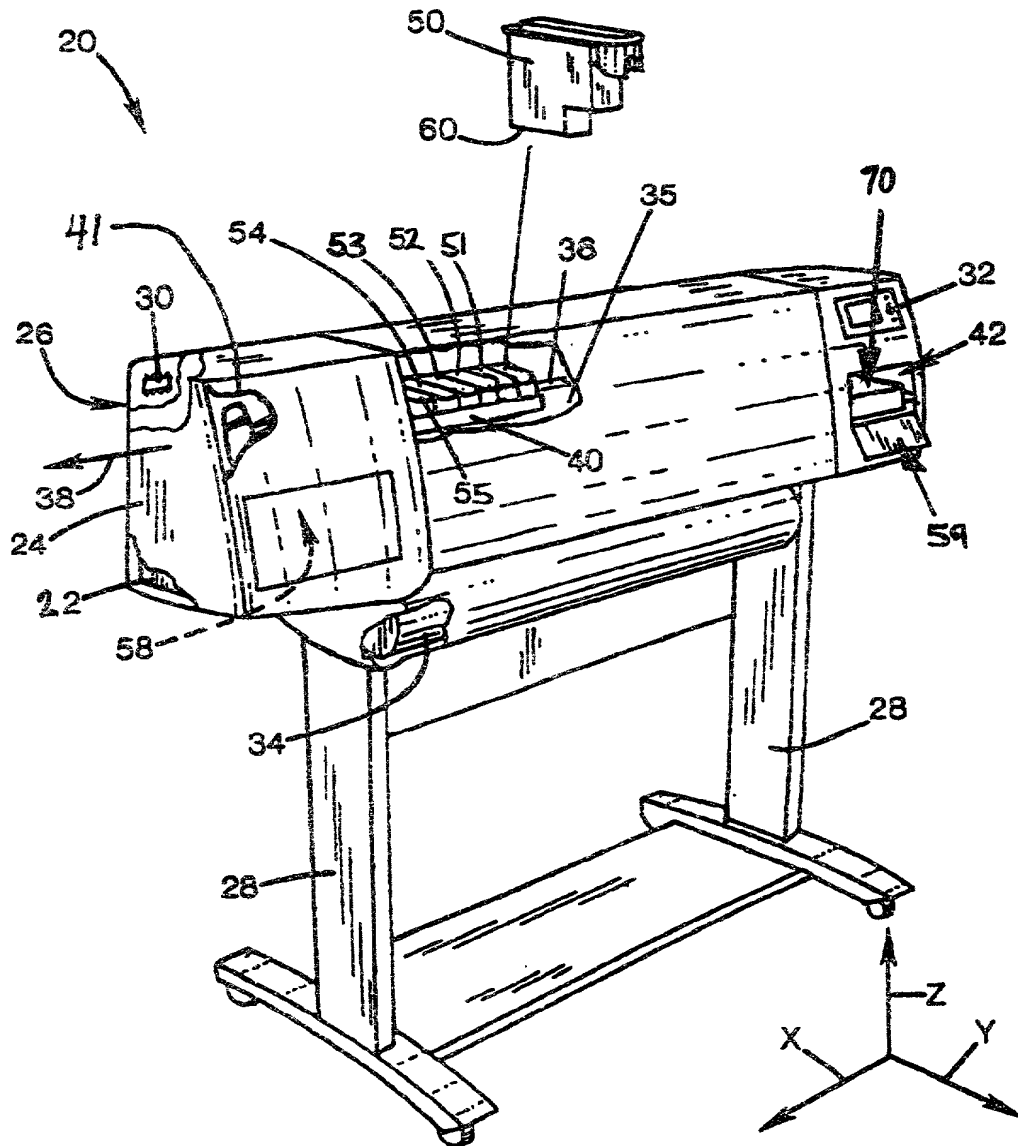


FIG. 2

FIG. 2

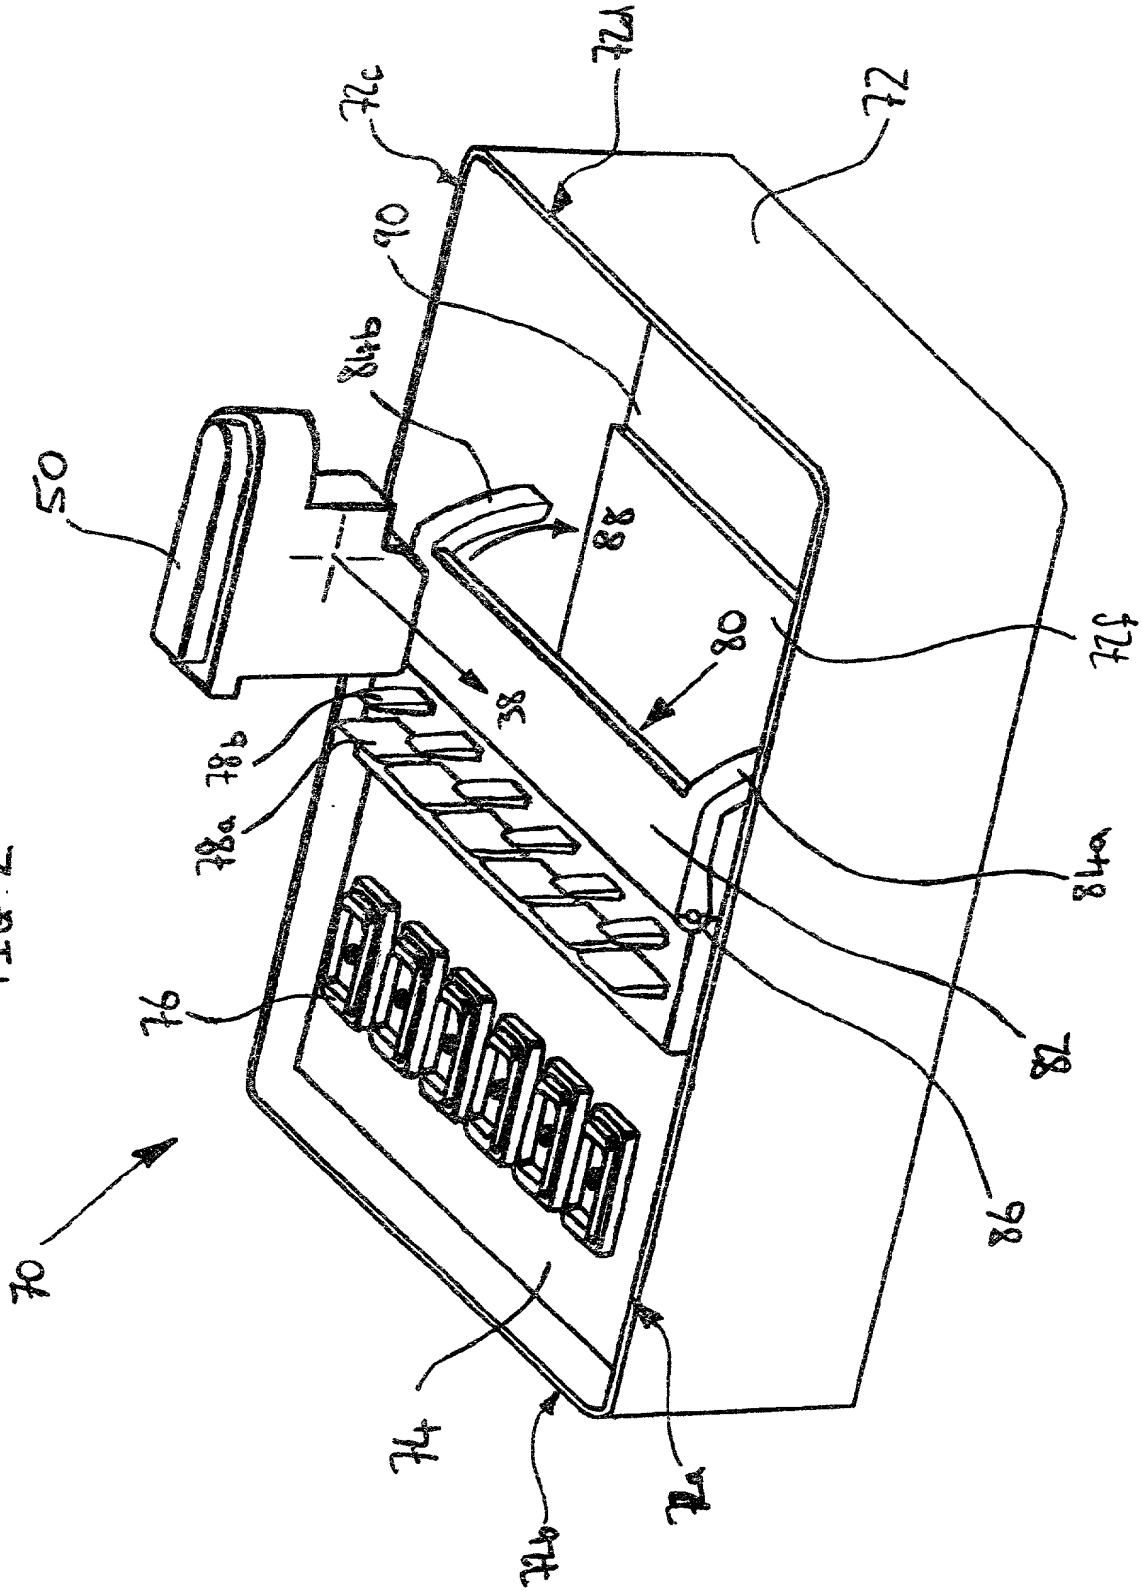

MS 44

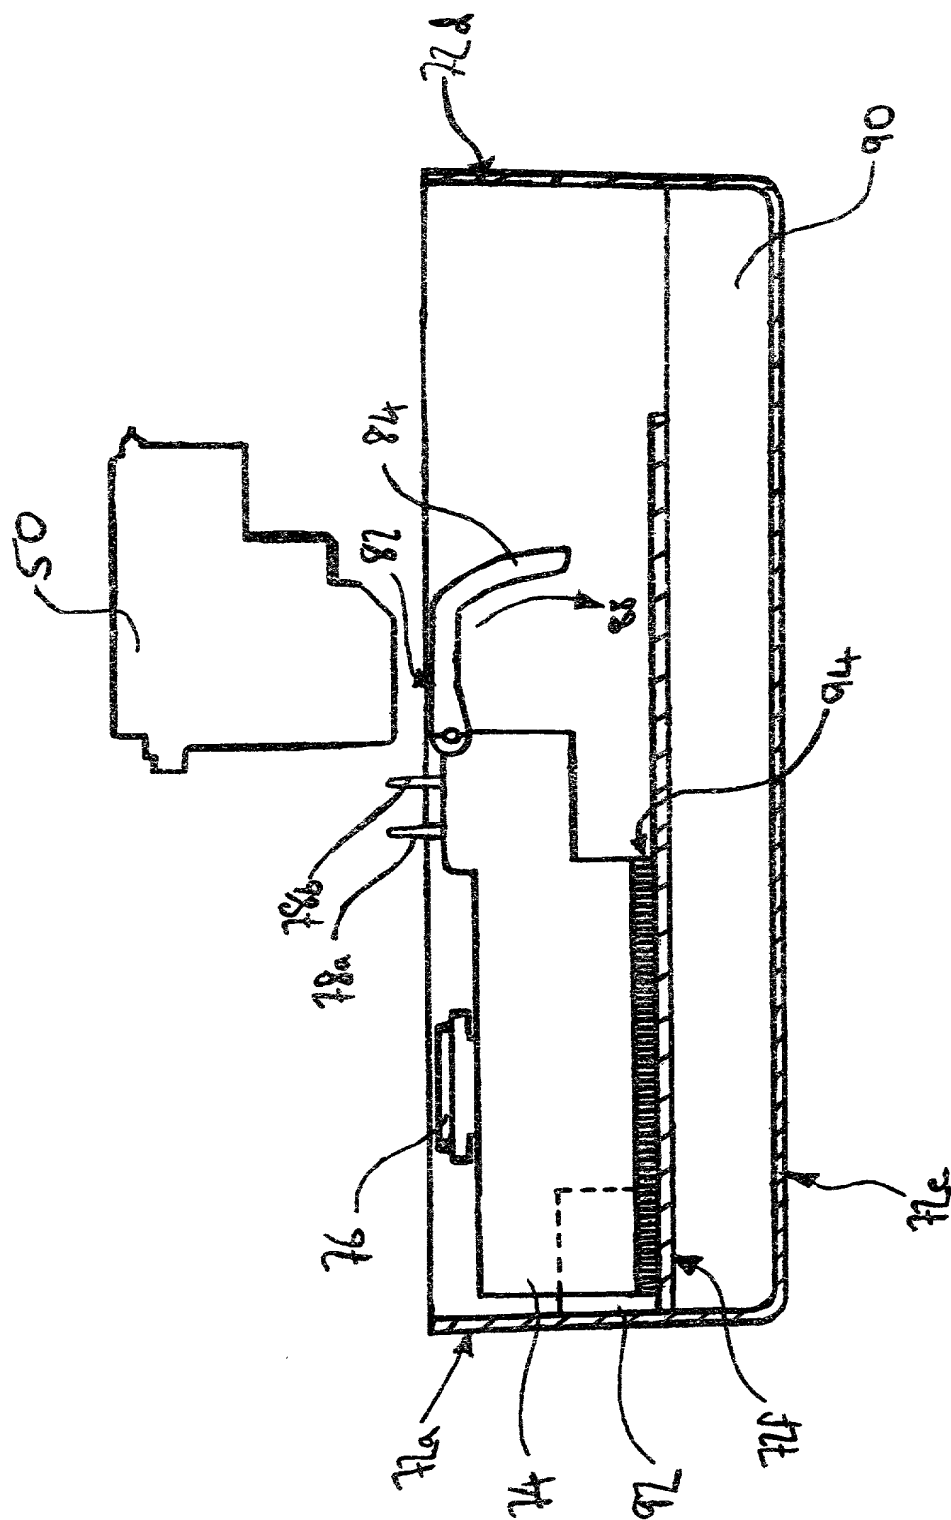
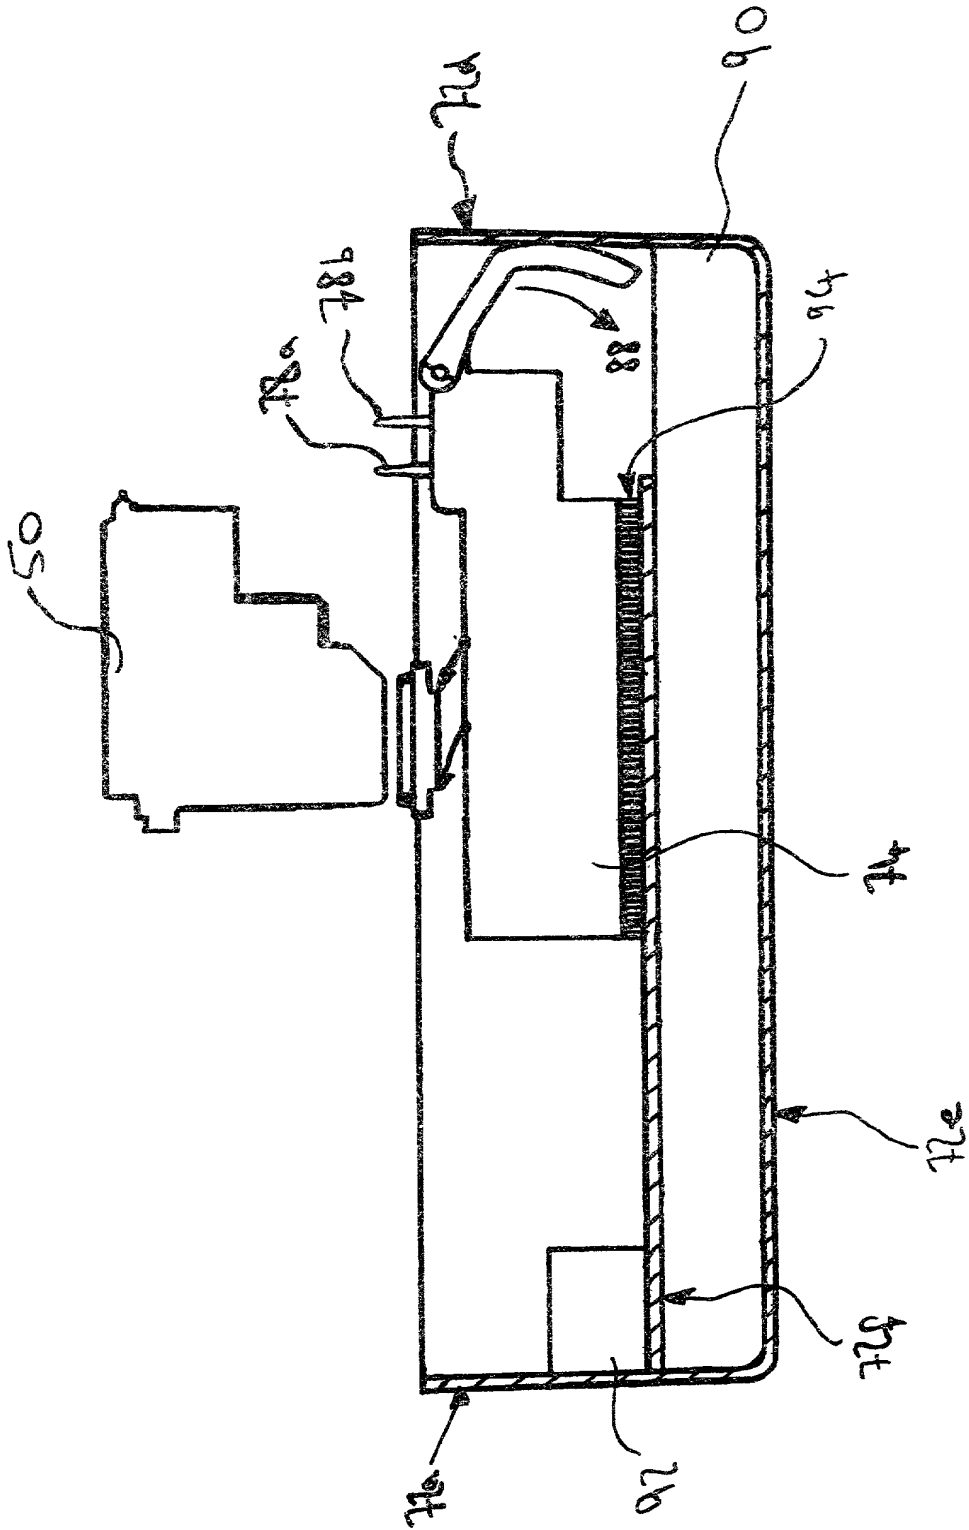


FIG 3b



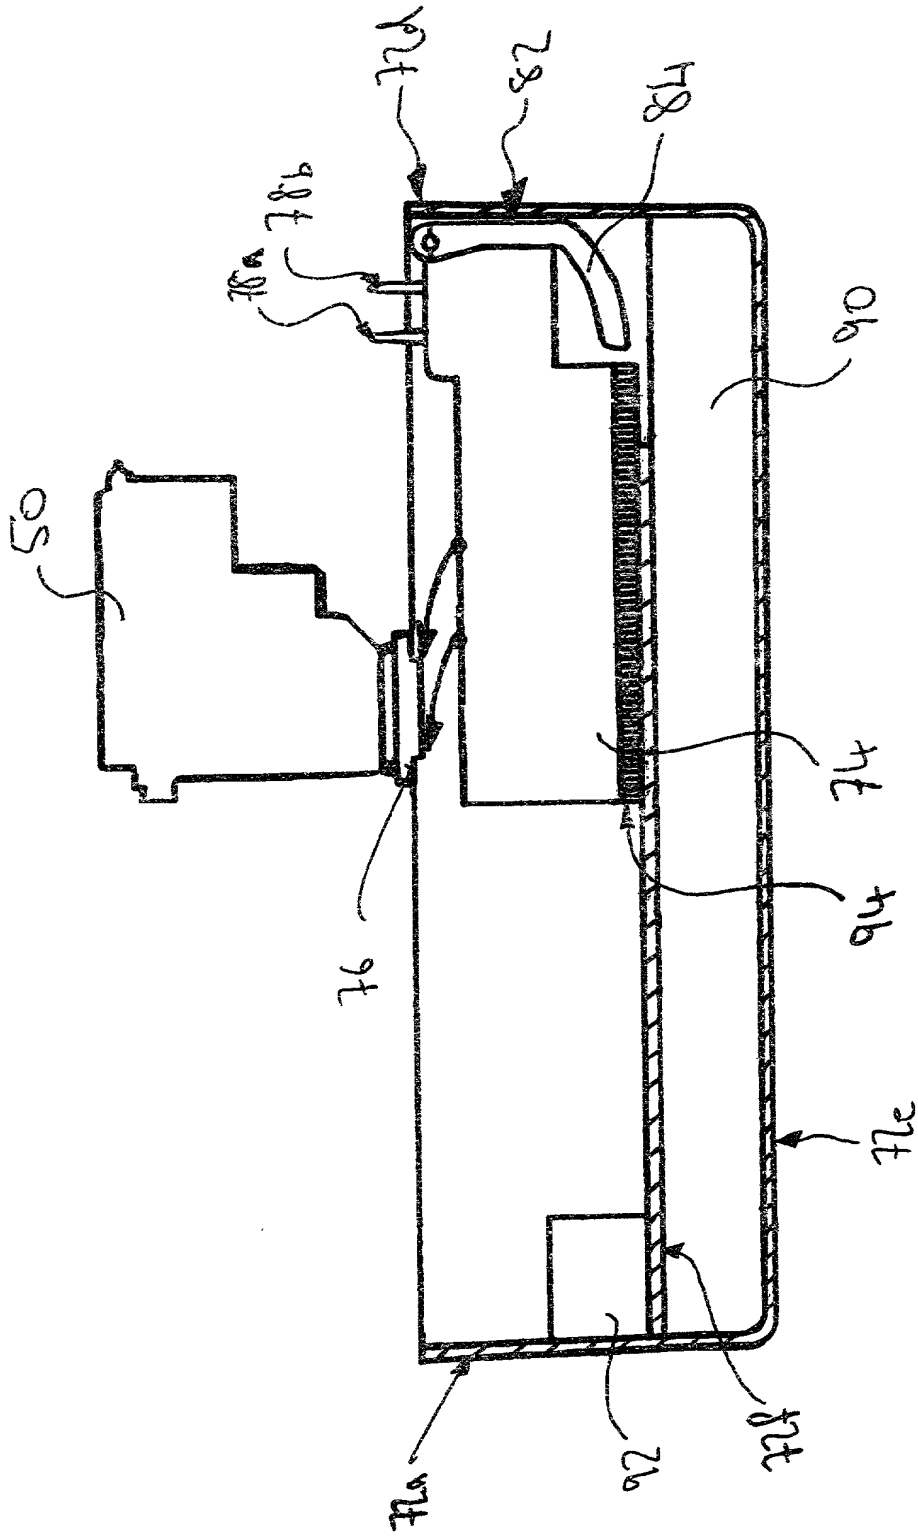


FIG 4

FIG 4 is a cross-sectional view of the device.

